




DNA  
DIAGNOSTIC

# User Manual Pneumo 4VC55

RNA extraction – cDNA synthesis - qPCR - Interpretation



**USER MANUAL**  
Cat No. PN4VC55  
DNA Diagnostic A/S  
[www.dna-diagnostic.com](http://www.dna-diagnostic.com)  
Revision 2019.06.19

## TABLE OF CONTENTS

1. PURPOSE OF THE TEST .....	3
2. PRINCIPLE OF THE TEST .....	4
3. KIT COMPONENTS AND STORAGE .....	5
4. REQUIRED EQUIPMENT AND MATERIALS NOT INCLUDED IN THE KITS.....	6
5. PROTOCOL.....	7

### **Trademarks:**

Black Hole Quencher® (BHQ®) and CAL Fluor® dye technologies incorporated in this product are used under licensing agreement with Biosearch Technologies, Inc. and protected by U.S. and world-wide patents issued, or in application.

## **1. PURPOSE OF THE TEST**

Calf pneumonia is a major problem in dairy and beef herds worldwide because it can result in serious economic loss due to the direct costs of calf losses and treatment. Calf pneumonia can be viral or bacterial in origin, but most often an initial viral infection is followed by a bacterial infection.

Pneumo 4VC55 is a fast, reliable and easy-to-use method for the detection of the primary viral pathogens (Bovine parainfluenza virus, Bovine coronavirus, Bovine Respiratory Syncytial virus, Bovine viral diarrhea virus and Bovine Herpesvirus 1) linked to calf pneumonia. Using a simple 96 deepwell-based extraction protocol followed by a sensitive and highly specific RT-qPCR reaction, the entire protocol from RNA extraction to result can be carried out in 5 hours.

## 2. PRINCIPLE OF THE TEST

Pneumo4VC55 allows the detection of Bovine parainfluenza virus, Bovine coronavirus, Bovine Respiratory Syncytial virus, Bovine viral diarrhea virus and Bovine Herpesvirus 1 in tracheal aspirate fluid sample from calves. It includes the following four main steps:

The RNA extraction step uses the Pneumo 4 Extraction Kit for RNA extraction from 0.5 mL of sample. The sample is incubated with pre-lysis buffer at 37 °C for 10 minutes and then spun and washed. The RNA is extracted by incubating sample in the lysis mix buffers at 37 °C for 20 minutes followed by 95°C for 15 minutes and debris is pelleted by centrifugation. Now the RNA is in the supernatant.

The cDNA synthesis step uses 5 µL of RNA template which is added to a well in a 96 well plate containing ready to use cDNA master mix. The cDNA synthesis reaction runs for 1 hour and 15 minutes.

The PCR step uses 2 µL of cDNA template which is added per well in a 96 well plate containing Pneumo4VC55 qPCR master mix. The qPCR reaction run for approximately 52 minutes. Each qPCR reaction contains four sets of primers and fluorescence probes for specific detection of five viruses. A fifth set of primers and probe detects an internal amplification control (IAC). Each of the four probes emit a specific light (color) enabling the identification of viruses present in the sample. Probes with CY5, ROX, HEX and FAM fluorophores are present for detection of Bovine parainfluenza virus, Bovine coronavirus, Bovine Respiratory Syncytial virus and Bovine viral diarrhea virus/Bovine Herpesvirus 1 amplicons, respectively. The tests use the standard 96 well plate format and ready-to-use reaction mixes. The test requires only pipettes, a vacuum aspirator, a centrifuge, incubation oven, a thermal heating block and a qPCR instrument.

The interpretation step involves inspection of the amplification plots. The functionality of the qPCR reaction is controlled by the presence of IAC amplicons resulting in an ATTO signal with a Ct value at 27-32. The CY5, ROX, HEX and FAM signals  $\leq 37$  show the sample is positive for Bovine parainfluenza virus, Bovine coronavirus, Bovine Respiratory Syncytial virus and Bovine viral diarrhea virus/Bovine Herpesvirus 1 amplicons, respectively. No Ct value shows that the sample is negative.

### 3. KIT COMPONENTS AND STORAGE

The Pneumo4VC55 kit contains material for testing 384 samples (cat. No. PN4VC55).


**The Pneumo4VC55 kit contains one box** for storage at room temperature (RT) and **two box** for storage at -20°C:

BOX	COMPONENTS	AMOUNT	STORAGE
		cat. No. PN4VC55	
I	Sealed 96 Deep Well Plates containing pre-lysis solution	4 x 96 Deep Well Plate	RT
	Wash Buffer	4 bottle of 110 mL	RT
	96 Well Plates (0.2 mL clear tubes) with cap	4 x 96 well plate (0.2 mL clear tubes) with cap	RT
	Adhesive seals for Deep Well plates	16 pieces	RT
	Cap mats for the qPCR 96 Well Plates	4x 96 cap for qPCR tube	RT
II	Lysis Buffer-I	2 bottle of 12 mL	-20°C
	Mix I Additive for Lysis Buffer-I	2 tube of 1334 µl	-20°C
	Sealed 96 Well Plates (0.2 mL white tubes) with Pneumo 4VC55 qPCR Master Mix	4 x 96 well plates	-20°C
III	Sealed 96 Well Plates (0.2 mL clear tubes) with cDNA Master Mix I	4 x 96 well plates	-20°C

#### 4. REQUIRED EQUIPMENT AND MATERIALS NOT INCLUDED IN THE KITS

- Centrifuge for 96 well plates. Centrifuge **must be capable of running at 5000 x g at 37°C**.  
*Example: Heraeus Multifuge X3R Centrifuge with HIGHPlate 6000 rotor.*
- Incubator at 37°C.
- Vacuum system or plate washer capable of aspirating supernatant from Deep Well plates.  
*Example: Vacuum system connected to an 8-channel adaptor (contact DNA Diagnostic for information) or vacuum system with pipette tips (35mm from tip to rim stop).*
- qPCR instrument e.g Biorad CFX96 touch with filters for QUASAR705 (440nm-492nm), FAM (492nm-516nm), HEX (535nm-555nm), Texas Red (585nm-610nm), CY5 (635nm-665nm).
- Vortexer for 96 well plates.
- Ice bucket or 0-4°C cooling block.
- Standard lab pipettes and sterile filter tips.

## 5. PROTOCOL

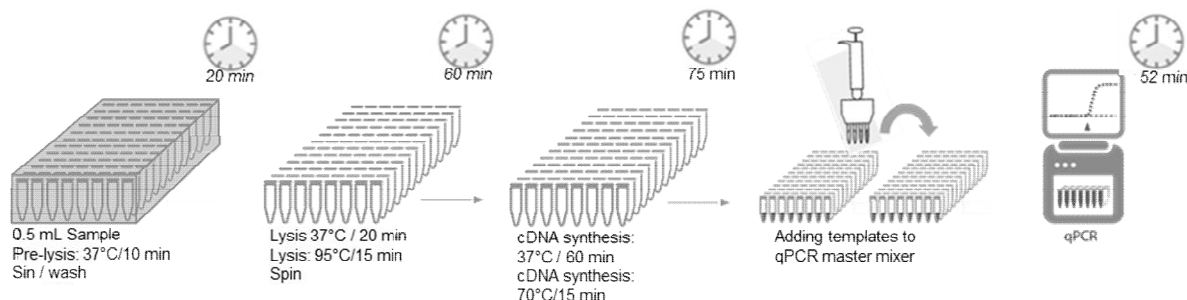

### RNA extraction:

1. Centrifuge a 96 Deep Well Plate containing 150  $\mu$ L of pre-lysis buffer at 1000 xg for 1 minute and remove seal.
2. Transfer 0.5 mL of samples to the corresponding well of the 96 well plate with pre-lysis buffer.
3. Pipette briefly up and down to mix the sample and cover wells with seal.
4. Incubate at 37°C for 10 minutes.
5. Spin Deep Well plate at 5000 xg for 5 minutes at 37°C.
1. Remove supernatant with a vacuum system or plate washer. It is important to remove the supernatant completely. Be careful not to touch or remove the pellets.  
*Note: It is important to remove all supernatant from the pellet. Therefore, correct adjustment of the plate washer syringes is required.*
2. Add 1 mL Wash Buffer to Deep Well plate.
3. Cover wells with seal and vortex briefly.
4. Centrifuge the plate at 5000 xg for 5 minutes.
5. Remove supernatant with a vacuum system or plate washer. It is important to remove the supernatant completely. Be careful not to touch or remove the pellets.
6. Prepare fresh Lysis-I Mix by adding 6  $\mu$ L Mix I additive to 54  $\mu$ L Lysis buffer-I.

Lysis-I Mixer	1 reaction	9 reaction	50 reaction	100 reactions
Lysis Buffer-I	54 $\mu$ L	486 $\mu$ L	2700 $\mu$ L	5400 $\mu$ L
Mix I additive	6 $\mu$ L	54 $\mu$ L	300 $\mu$ L	600 $\mu$ L
Total	60 $\mu$ L	540 $\mu$ L	3000 $\mu$ L	6000 $\mu$ L

7. Add 60  $\mu$ L Lysis-I Mix, to each pellet. Vortex and spin 20 seconds at 1000 xg to bring Lysis mixer to the bottoms.
8. Transfer of 60  $\mu$ L from each sample into the corresponding tubes in the 96 well plate (clear 0.2 mL) and close the tubes with the caps. Avoid cross contamination.
9. Incubate the 96 well plate at 37°C for 20 minutes and at 95°C for 15 minutes.
10. Cool the 96 well plate on ice for 5 minutes

*Note: The incubation at 37°C and 95°C can be done using a PCR instrument programmed: 37°C for 20 min. → 95°C for 15 min. → 4°C for 5 minutes.*

11. Centrifuge the plate at 5000 xg for 5 minutes.
12. Carefully transfer 5 µL of each aqueous phase directly to the corresponding well of the 96 well plate with cDNA Master Mix in step 20.  
*Note: Due to the instability of RNA, it is recommended to perform the cDNA synthesis before storing samples.*

#### **cDNA Synthesis:**

13. Take a cDNA master mix plate from freezer and thaw it on ice. Briefly spin the plate to collect the cDNA master mix in the bottom.
14. Remove and discard the seal from cDNA master mix plate.
15. Carefully transfer 5 µL supernatant from the 96 well 0.2 mL plate (step 17) to the corresponding well in the cDNA master mix plate (clear 0.2 mL).
16. Incubate the cDNA reaction at 37°C for 60 minutes.
17. Inactivate Reverse Transcriptase enzyme by heating to 70°C for 15 minutes.
18. Cool the cDNA reaction tube on ice for 1 minute and spin it again for 1 minute to collect condensate.  
*Note: The cDNA samples can be kept at -20°C until use.*

#### **qPCR analysis:**

19. Take a Pneumo 4VC55 qPCR master mix plate (white 0.2 mL) from freezer and thaw it on ice. Briefly spin the qPCR plate to collect the qPCR master mix in the bottoms.
20. Remove and discard the seal from qPCR plate.
21. Carefully transfer 2 µL supernatant from the 96 well 0.2 mL plate (step 23) to the corresponding well in the Pneumo 4VC55 qPCR master mix plate.  
*Note: It is important to keep Master Mix on ice while loading template and to run the qPCR within 15 minutes.*
22. Carefully cover the qPCR reaction plate with new lids and spin at 1000-1500 xg for 30 seconds to 1 minute.
23. Insert qPCR plate into the qPCR instrument.
24. Run the qPCR reaction using the instrument setting and the running program below:



## Instrument settings for the CFX96 touch qPCR machine

Threshold settings:

Fluorophore	QUASAR705	FAM	HEX	Texas Red	CY5
Threshold	375	375	375	375	375
Baseline	“User defined” 10-15	“User defined” 10-15	“User defined” 10-15	“User defined” 10-15	“User defined” 10-15

The guidelines for setting baseline and threshold should be checked manually to ensure that threshold lines are in the exponentially area of the amplification plot and above the background.

*Baseline Correction.* Select “Baseline subtracted curve fit”.

Activate the following filters: FAM, HEX, Texas Red, Cy5 and QUASAR705.


### qPCR running program

Condition	Temperature	Duration	Number of cycles	Stage
Denaturation	95°C	1 min	1	Pre-incubation
Denaturation	*95°C	5 sec	40	Amplification
Annealing/extension	60°C	**25 sec		

*\*Only ramp rate should be set for 2.5 °C / sec without setting increment temp.*

*\*\* Read fluorescence for FAM, HEX, Texas Red, CY5, QUASAR705 at the end of each annealing/extension step.*

## Interpretation of analysis:

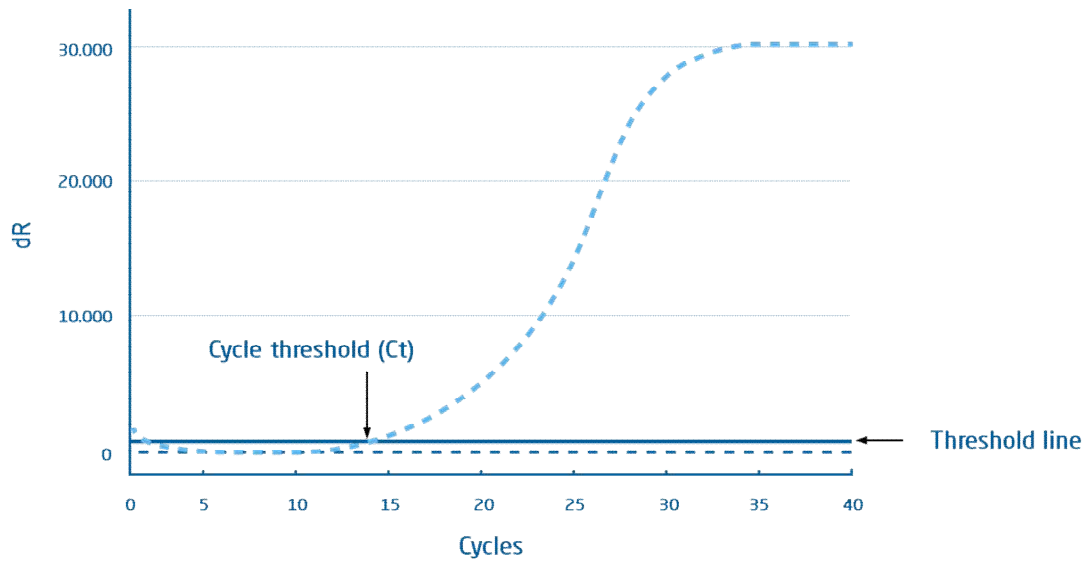

Amplification plot with the number of PCR cycles is shown on the x-axis, and the background subtracted fluorescence from the amplification reaction is shown on the y-axis. The threshold line is used to find the Ct value, where it intersects the amplification curve. Ct is optimally determined in the early exponential phase, when the fluorescence starts increasing due to PCR amplification. The threshold line is calculated automatically by the instrument giving in this example a Ct value of 14.

25. Check amplification plot for ATTO signals and the signals should be present in all reactions. The Ct must be in the interval 27-32 to confirm the qPCR reaction is functional.  
*Note: ATTO Ct can be above 32 or missing if the Ct for one or more of FAM, HEX, ROX, CY5 is low. Then the DNA sample should be diluted 5-10 times and a new qPCR reaction should be analyzed using this diluted DNA. A dilution of 10 times will theoretically move Ct values 3.3 higher. Reactions with no FAM, HEX, ROX, CY5 signal and ATTO signal absent or outside the interval 27-32 **must be retested**.*
  
26. Check amplification plot for CY5, ROX, HEX, FAM signals and interpret the results as described in the table below.

<b>Target</b>	<b>Filter</b>	<b>Positive</b>	<b>Negative</b>	<b>Retest</b>
		<b>Ct</b>	<b>Ct</b>	<b>Ct</b>
Bovine parainfluenza virus	CY5	≤37	>37 or absent	
Bovine coronavirus	ROX	≤37	>37 or absent	
Bovine Respiratory Syncytial virus	HEX	≤37	>37 or absent	
Bovine viral diarrhea virus and Bovine Herpesvirus 1	FAM	≤37	>37 or absent	
IAC	ATTO	≤32		>32 or absent

*Note: Sample with Ct values below 37 are considered as true positive.  
Sample with Ct values above 37 should be considered negative.*

**For more information, contact**

DNA Diagnostic A/S  
Voldbjergvej 14  
8240 Risskov  
Denmark  
Tel.: +45 8732 3050  
E-mail: [info@dna-diagnostic.com](mailto:info@dna-diagnostic.com)  
[www.dna-diagnostic.com](http://www.dna-diagnostic.com)

*DNA Diagnostic A/S was established in 1992. DNA Diagnostic A/S is an ISO 13485 certified developer, manufacturer, and worldwide supplier of PCR based in vitro diagnostic kits.*

**Cat. No.: PN4VC55**

**USER MANUAL**

■ ----- [www.dna-diagnostic.com](http://www.dna-diagnostic.com) ----- ►